






Pronation / Supination Inclinometer

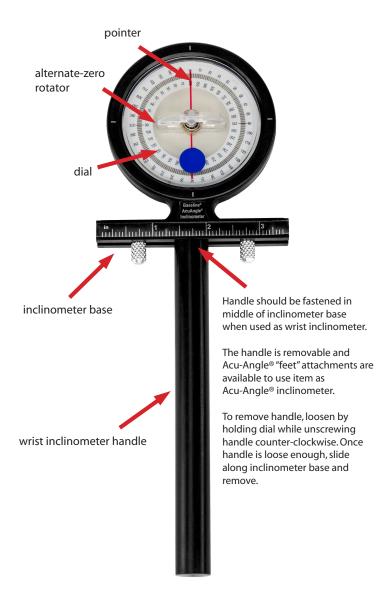


INSTRUCTIONS

Ensure that the handle attachment is securely fastened in the middle of the inclinometer base directly under the center of the dial.

- 1. (patient) Position arm and grip handle as instructed by therapist. Front of Dial (side with alternate-zero rotators) should face therapist.
- 2. (therapist) Stabilize patient's arm if necessary.
- 3. (therapist) Rotate dial to set "zero" to initial inclination.
- 4. (patient) Rotate wrist to either side as instructed by therapist.
- 5. (therapist) Note the maximum inclination achieved during trial.
- The maximum inclination is the range of motion measurement.








rev 0922



Pronation / Supination Inclinometer

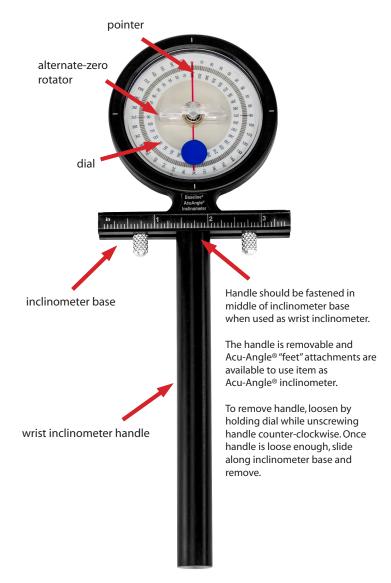

INSTRUCTIONS

Ensure that the handle attachment is securely fastened in the middle of the inclinometer base directly under the center of the dial.

- 1. (patient) Position arm and grip handle as instructed by therapist. Front of Dial (side with alternate-zero rotators) should face therapist.
- 2. (therapist) Stabilize patient's arm if necessary.
- 3. (therapist) Rotate dial to set "zero" to initial inclination.
- 4. (patient) Rotate wrist to either side as instructed by therapist.
- 5. (therapist) Note the maximum inclination achieved during trial. The maximum inclination is the range of motion measurement.







AJW Technology Consulting GmbH 40213 Düsseldorf (Germany)



